

FIG. 1A

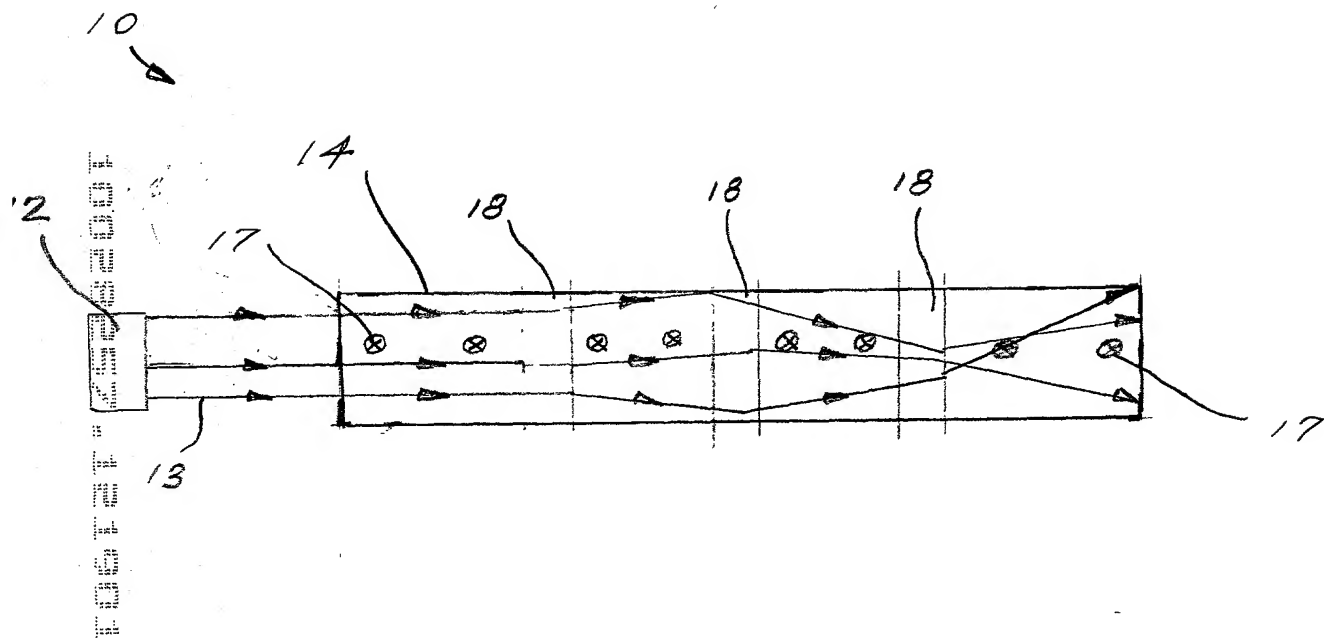
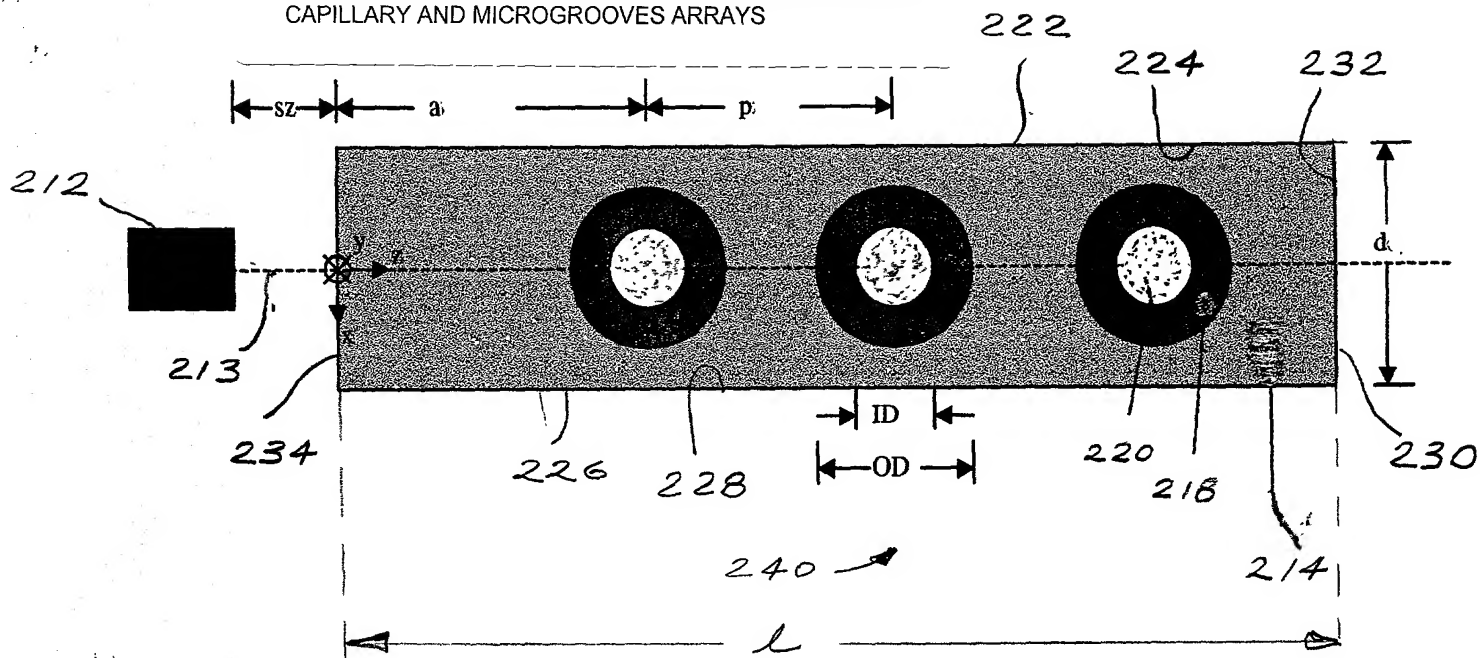
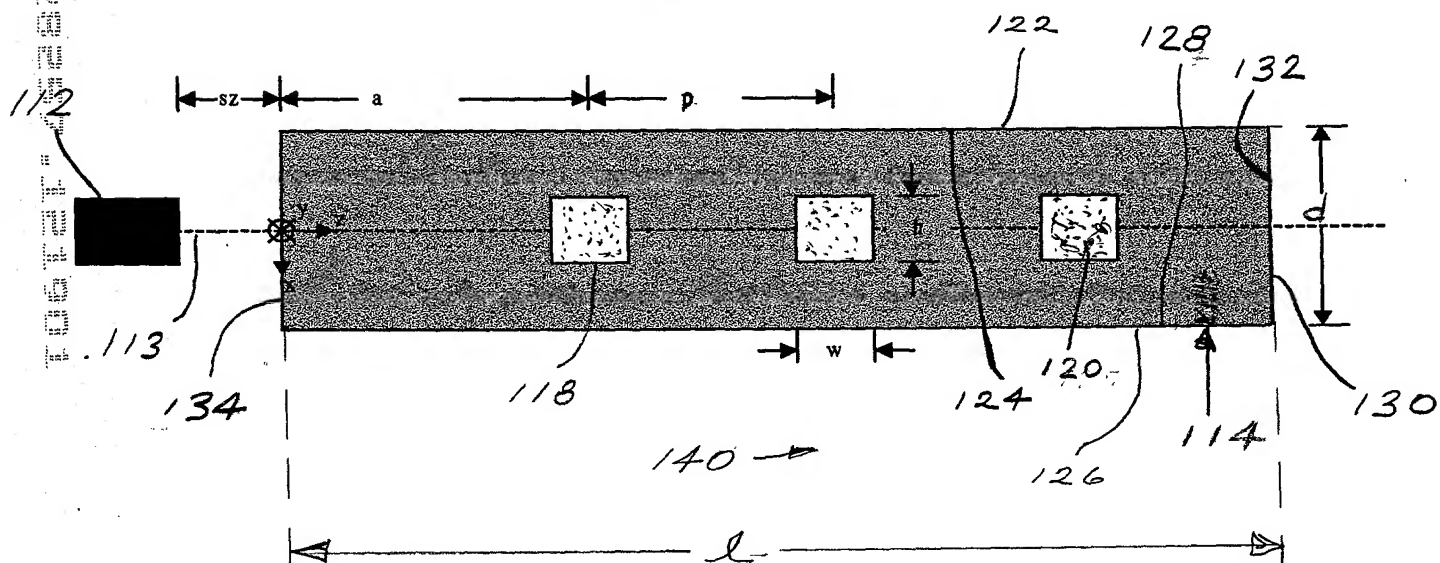
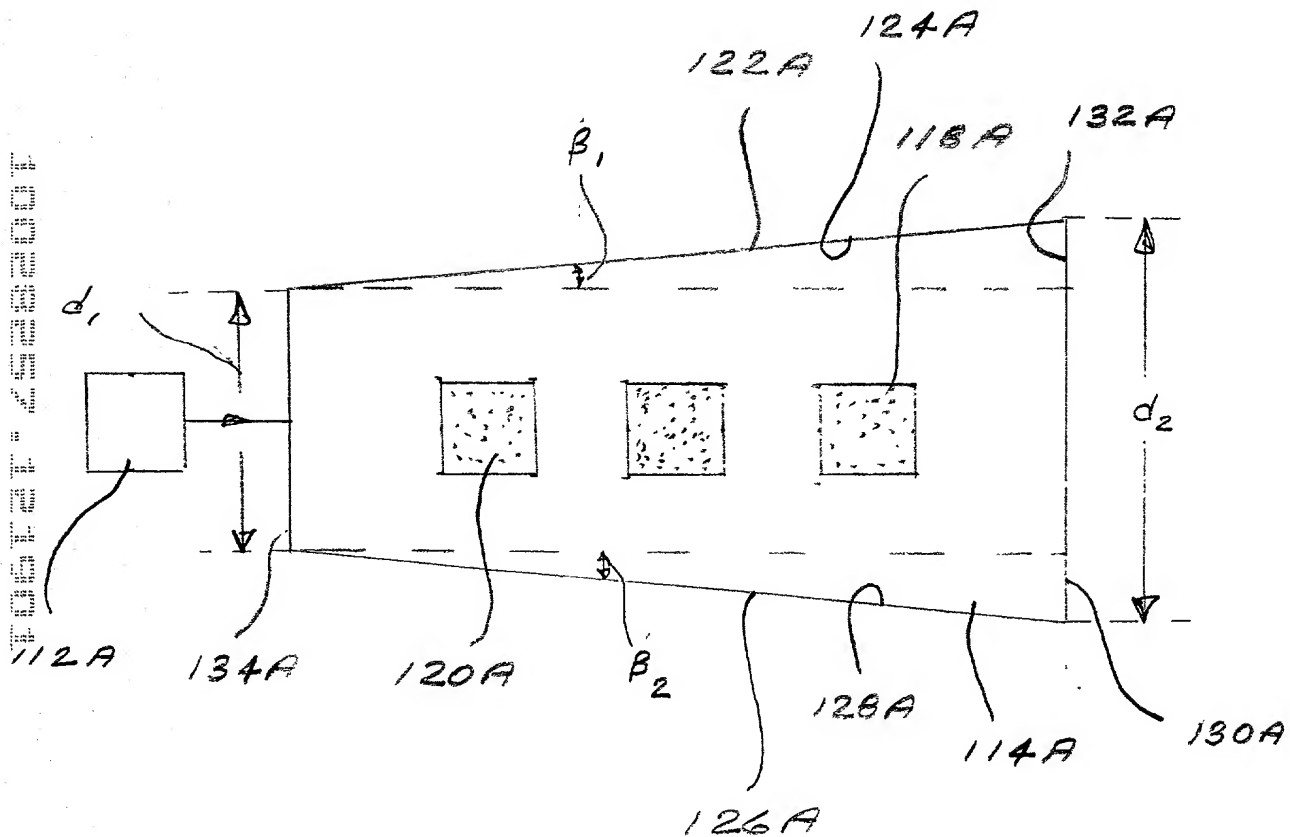


FIG. 1B

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYSFIG. 6FIG. 2A

FIG. 2B

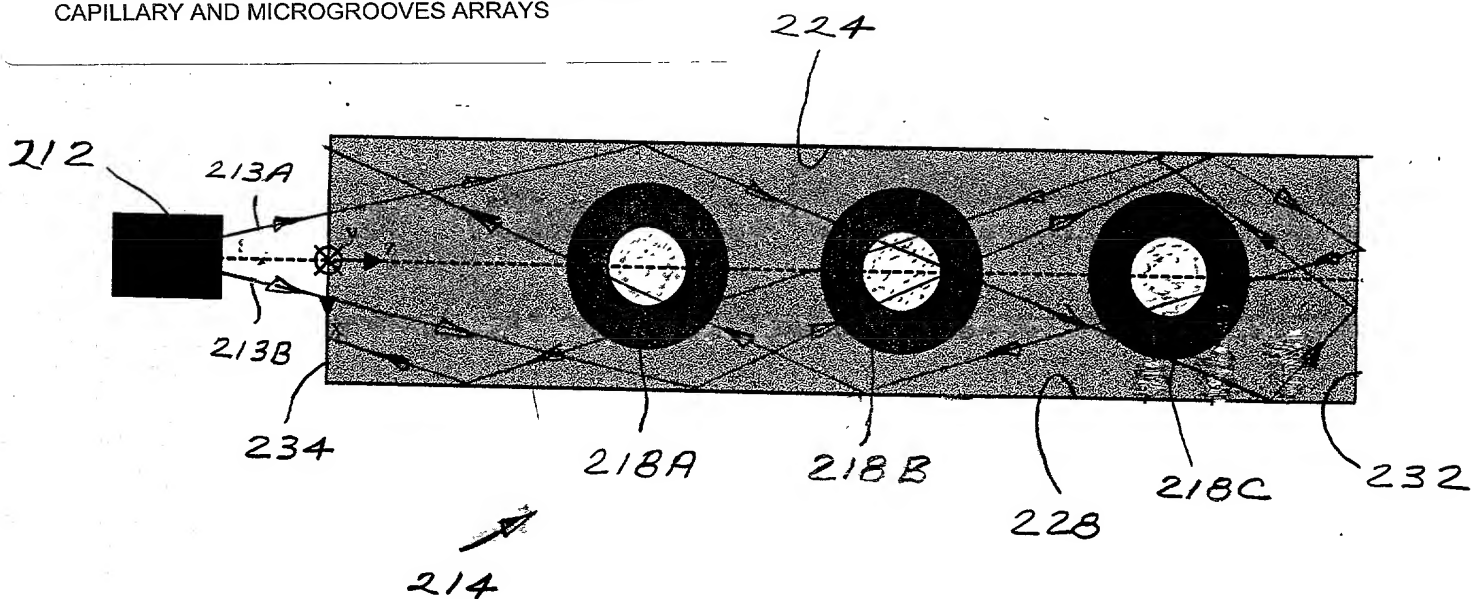


FIG. 7

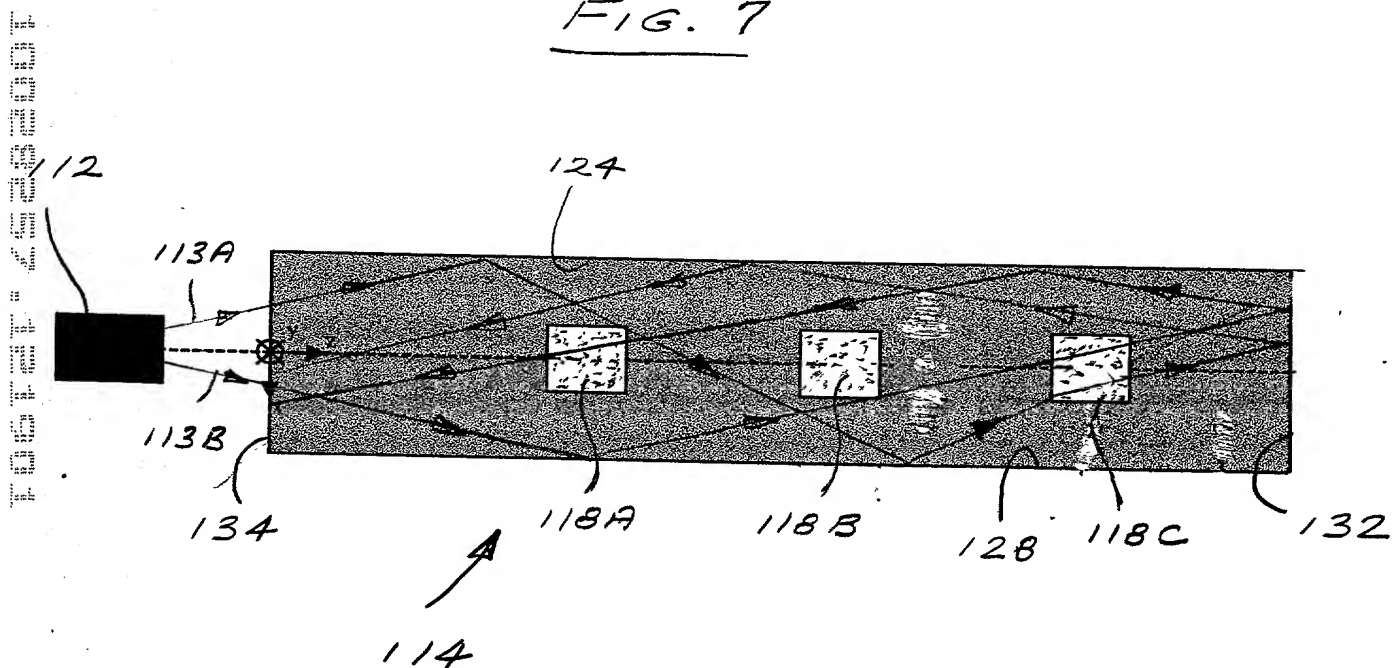


FIG. 3

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYS

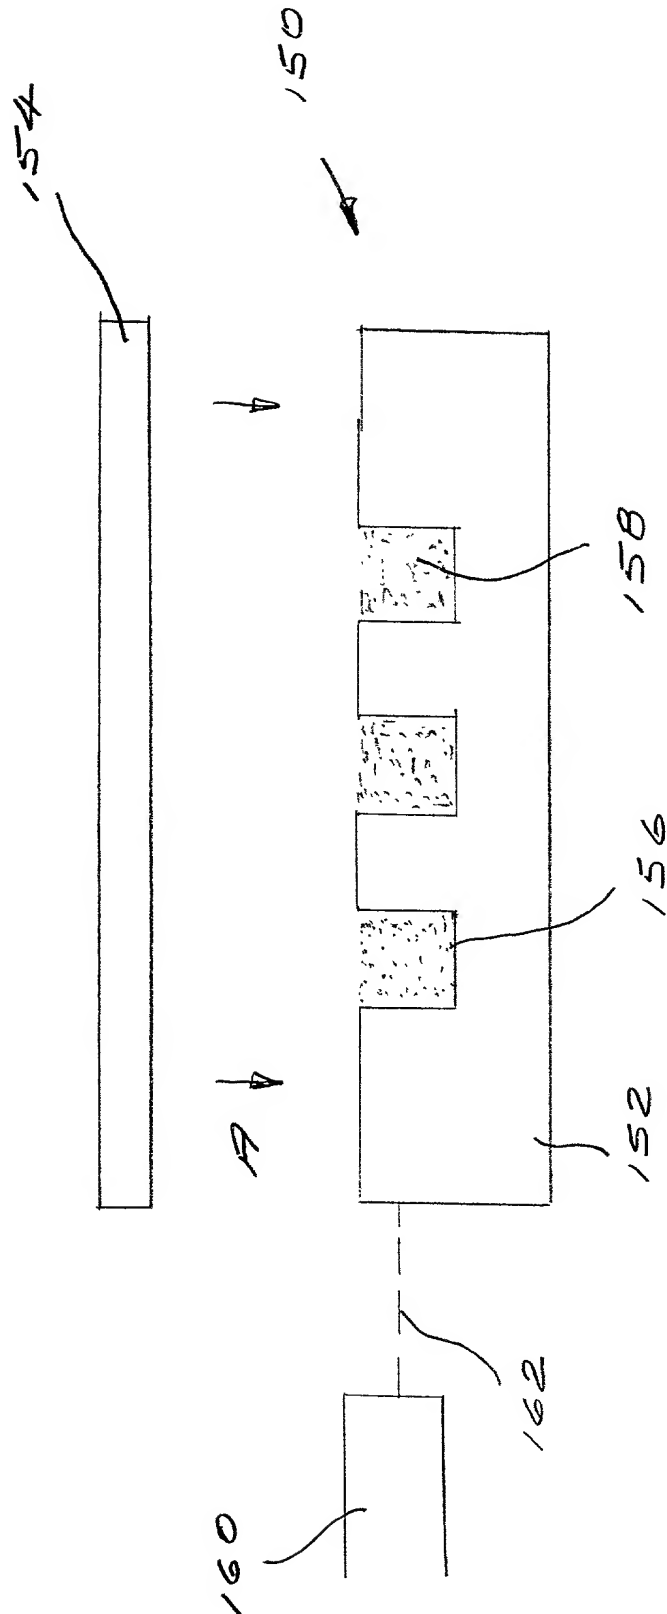


FIG. 4

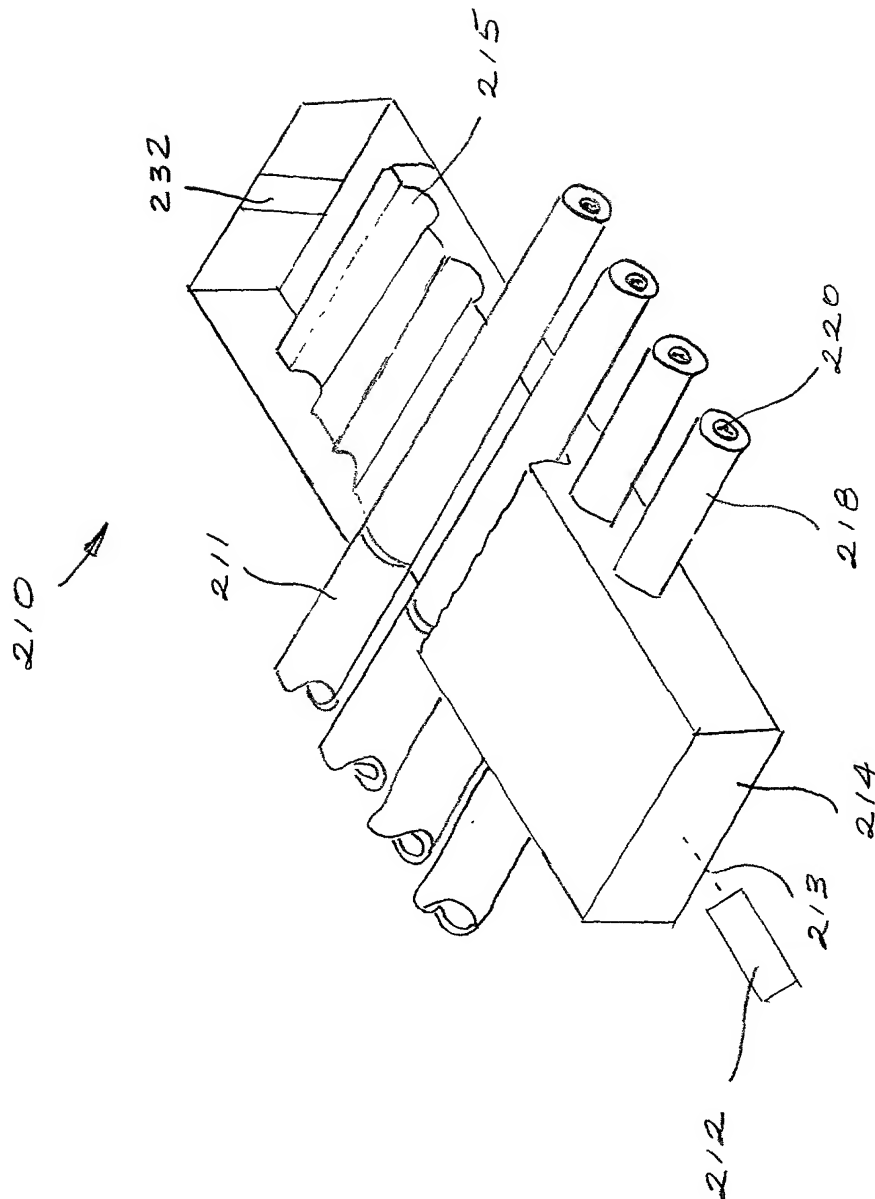


Fig. 5

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYS

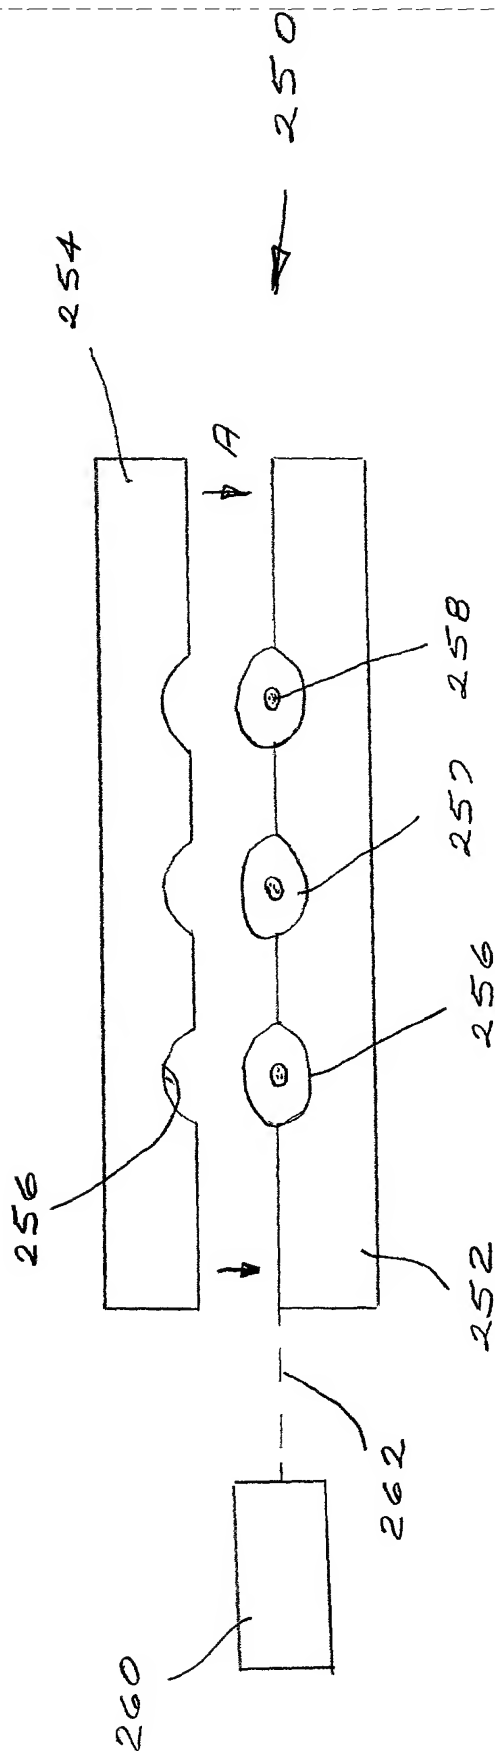


Fig. 8

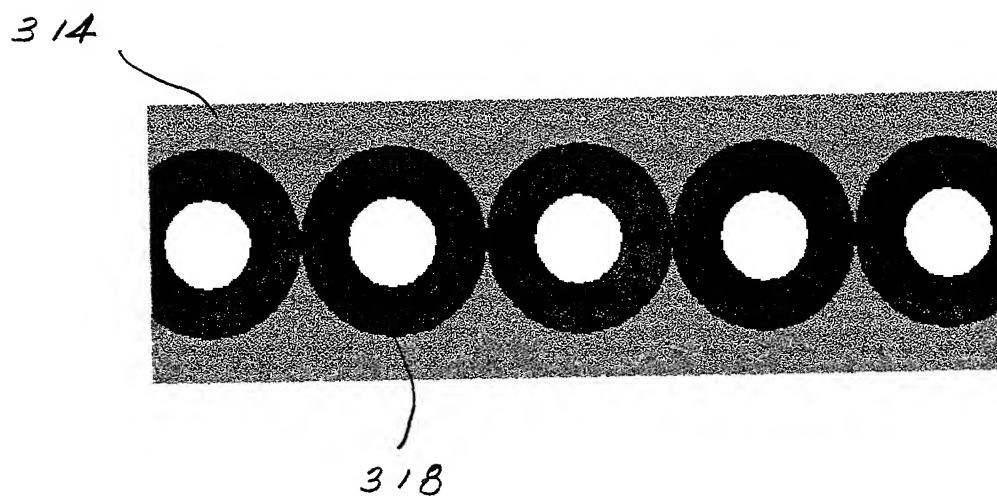


FIG. 9

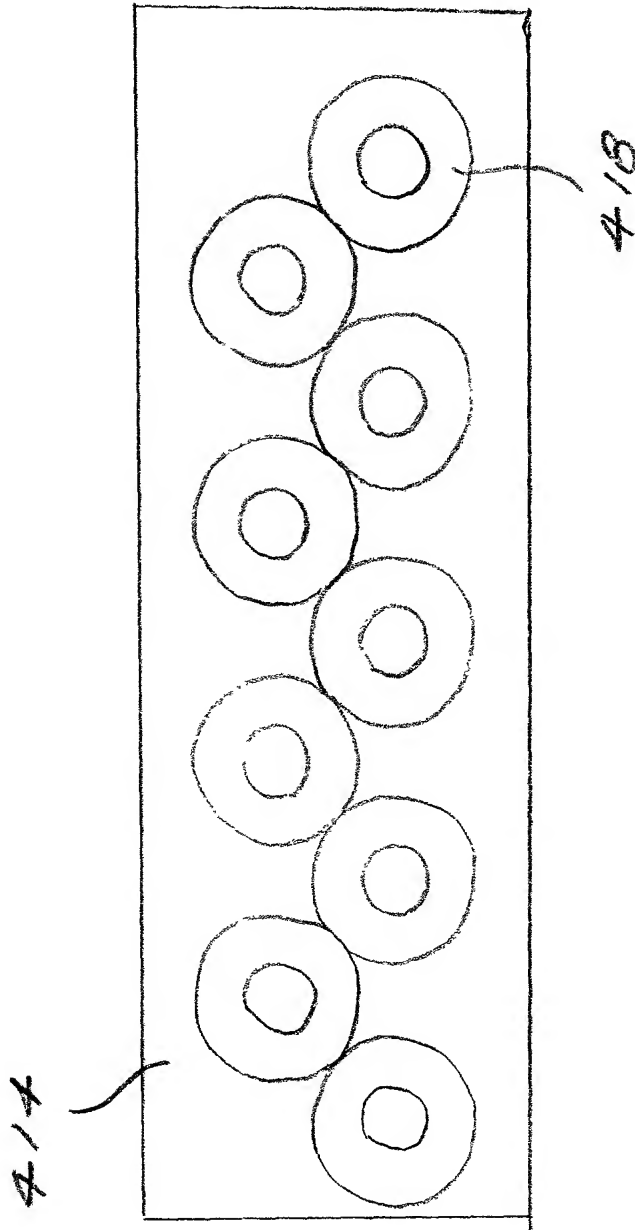


Fig. 10

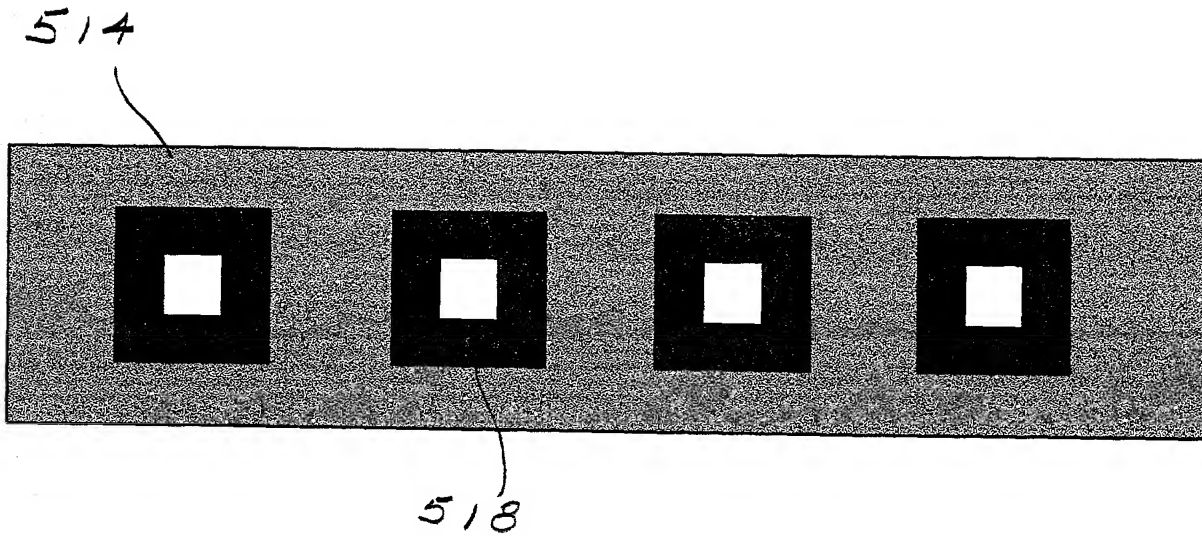


FIG. 11

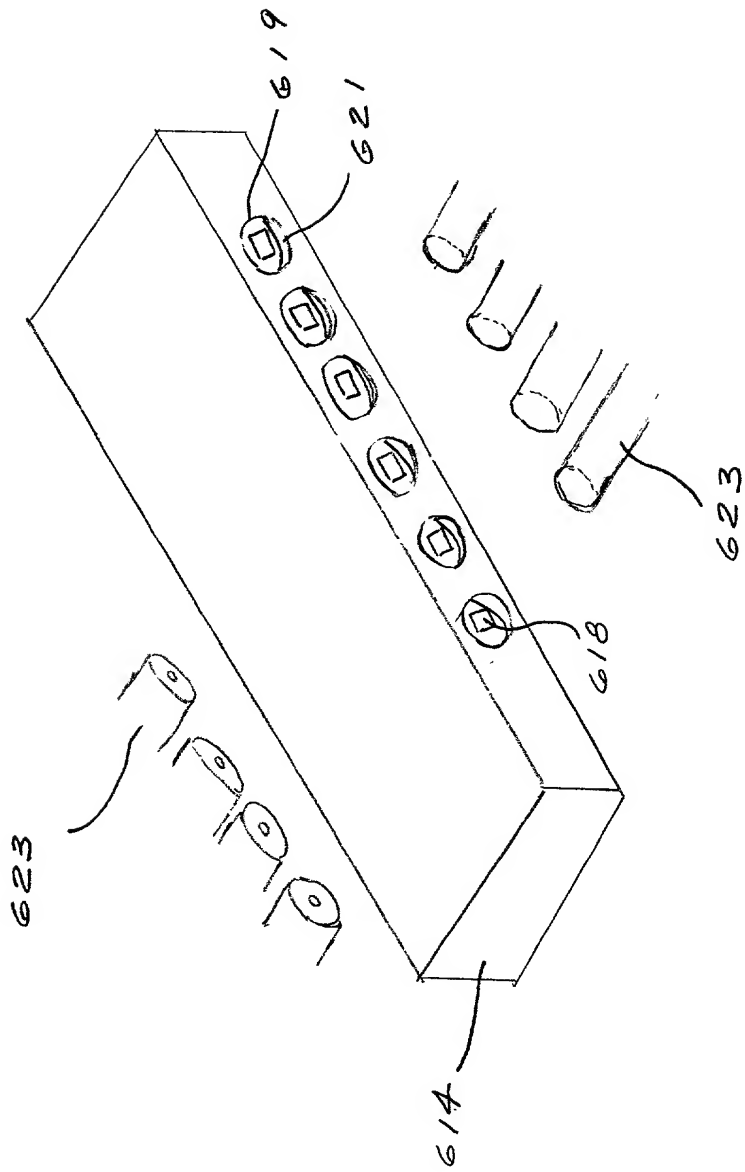
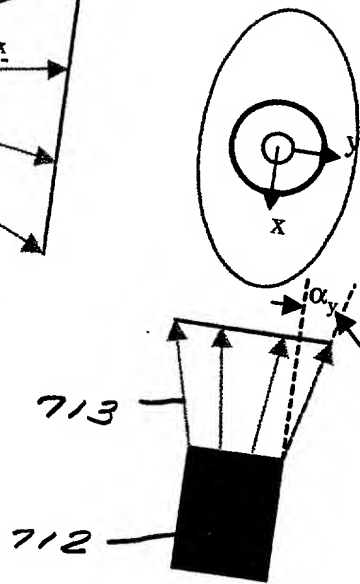
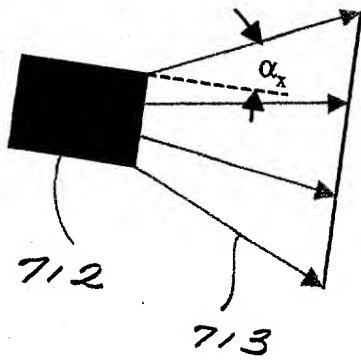


FIG. 12

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYS

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYS

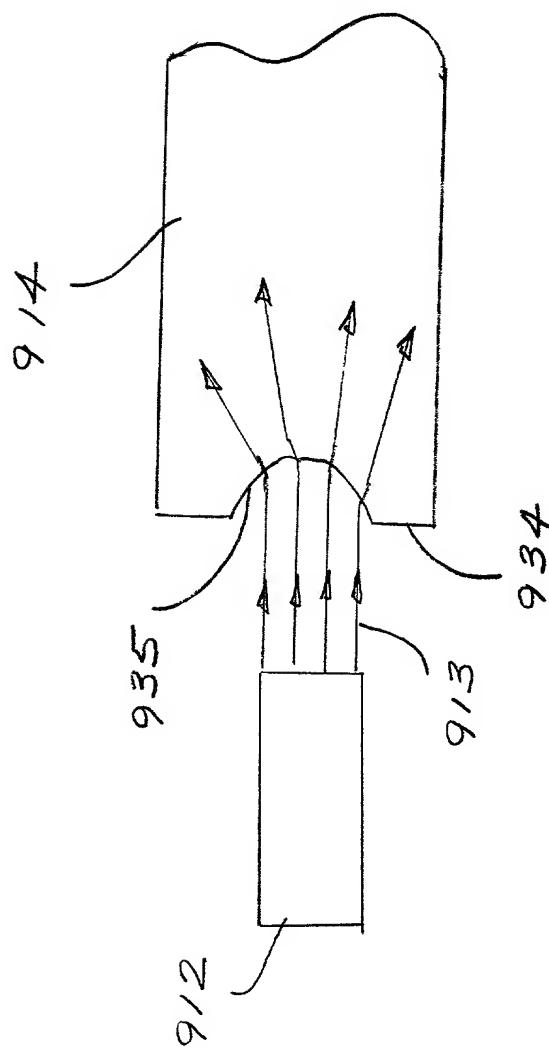


FIG. 14

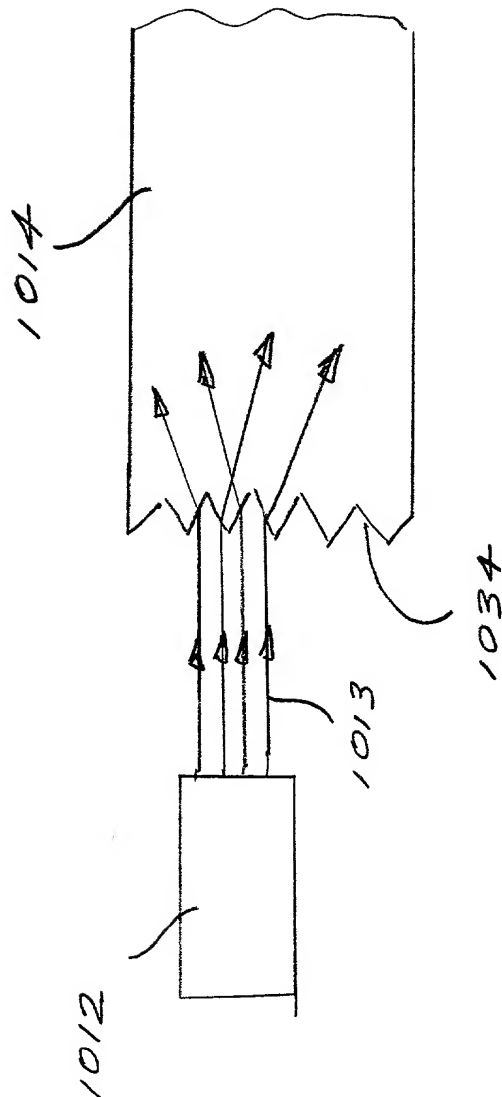


FIG. 15

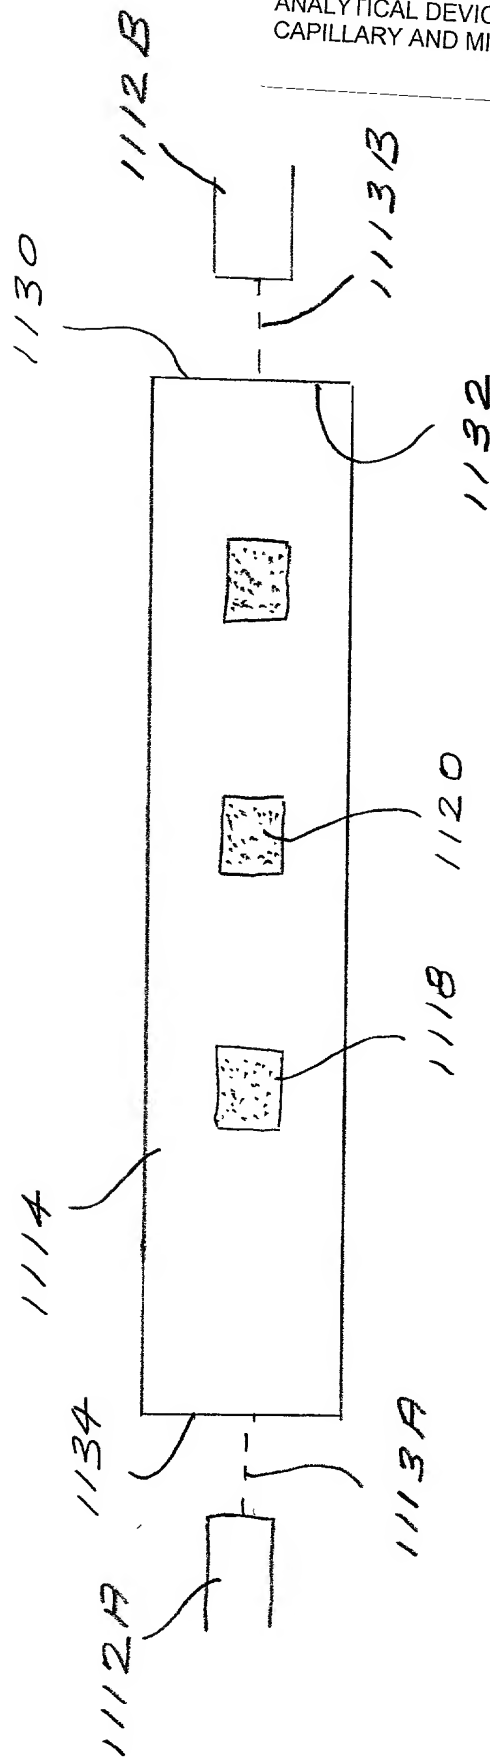


FIG. 16

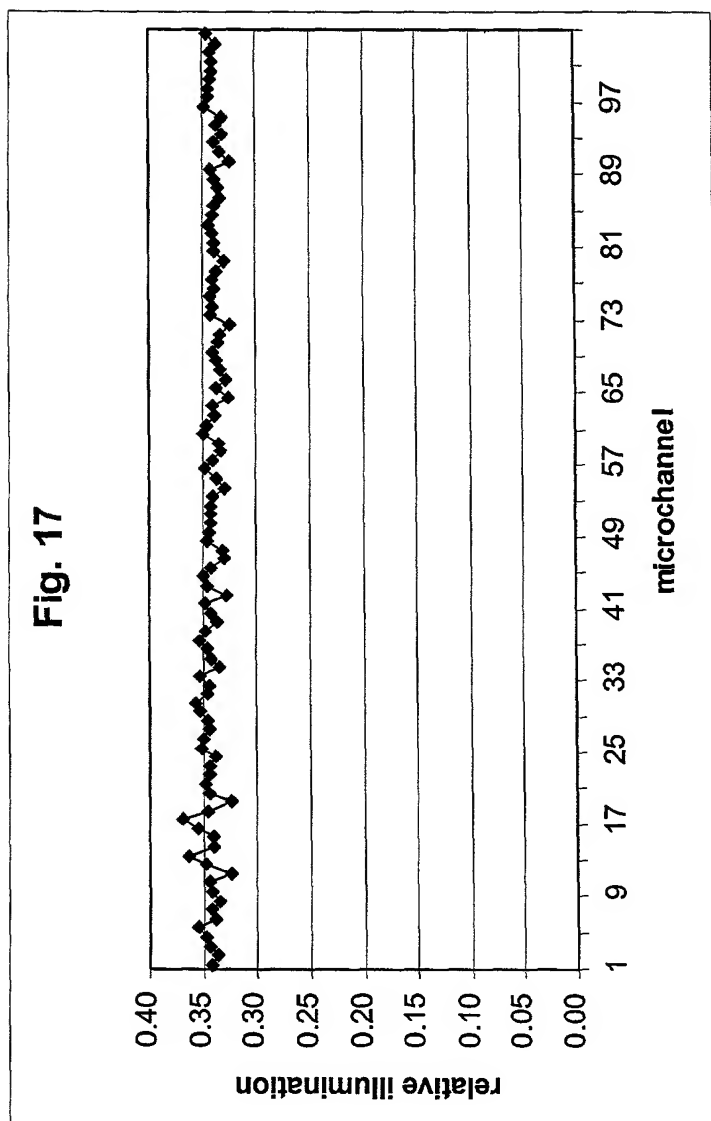
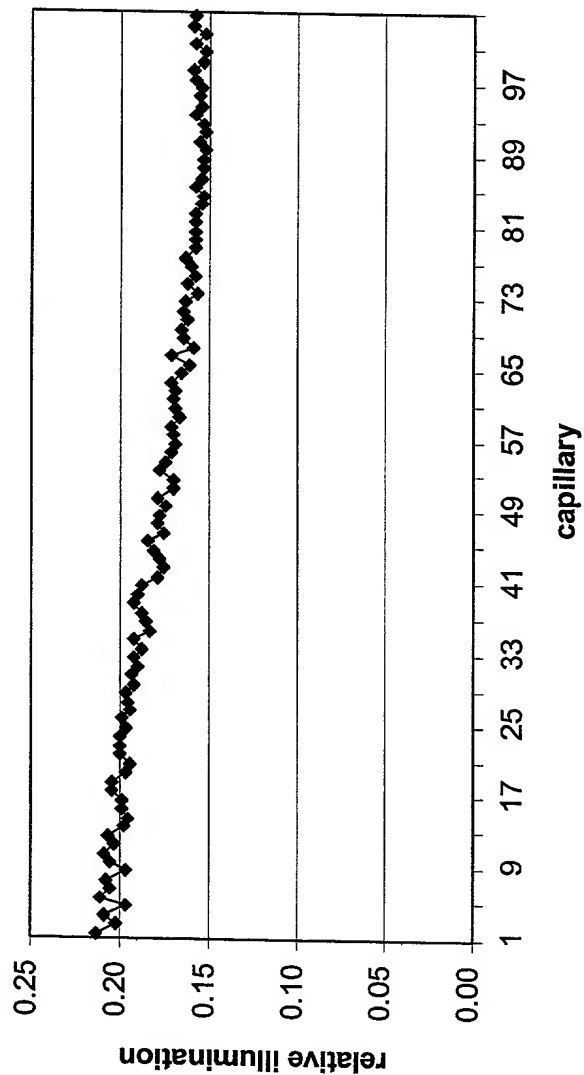


Fig. 18




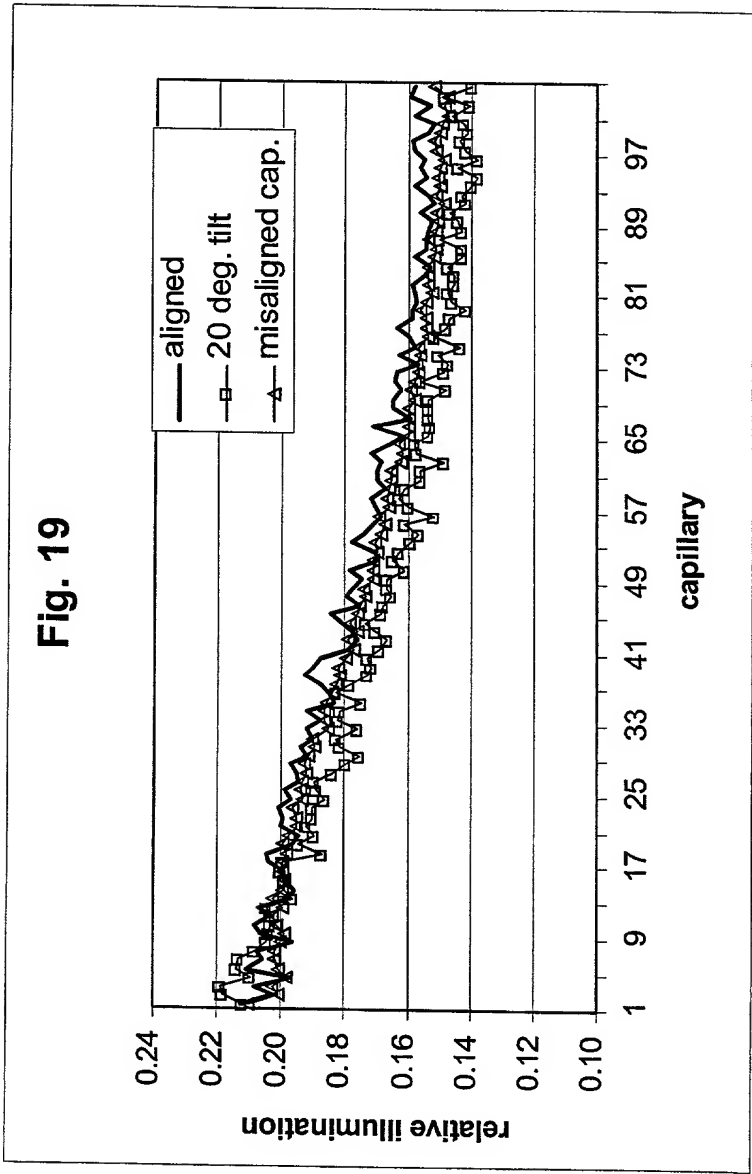


Fig. 20

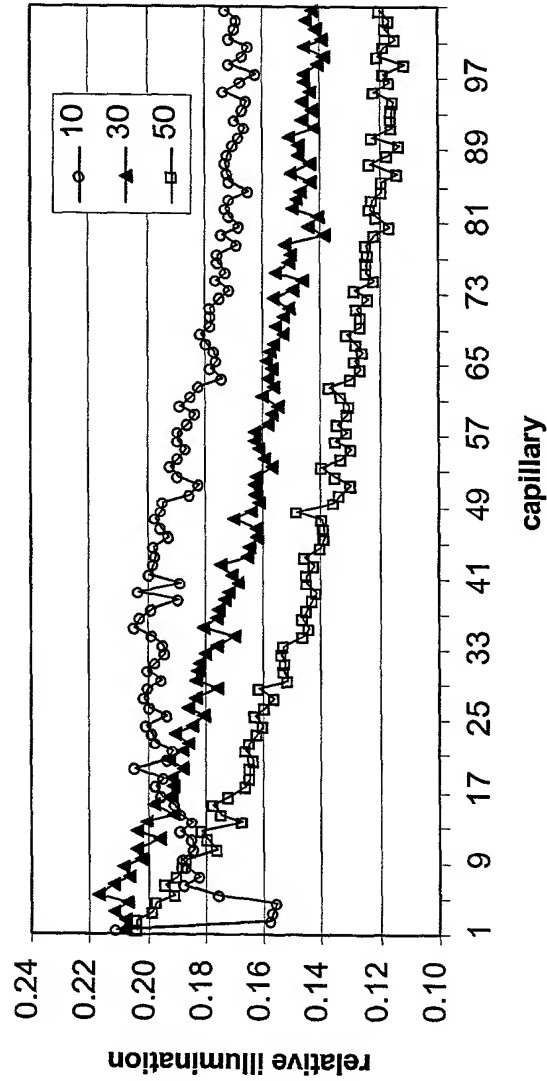

Applicant(s): Larry J. Carson et al.

ANALYTICAL DEVICE WITH LIGHTGUIDE ILLUMINATION OF
CAPILLARY AND MICROGROOVES ARRAYS

Fig. 21

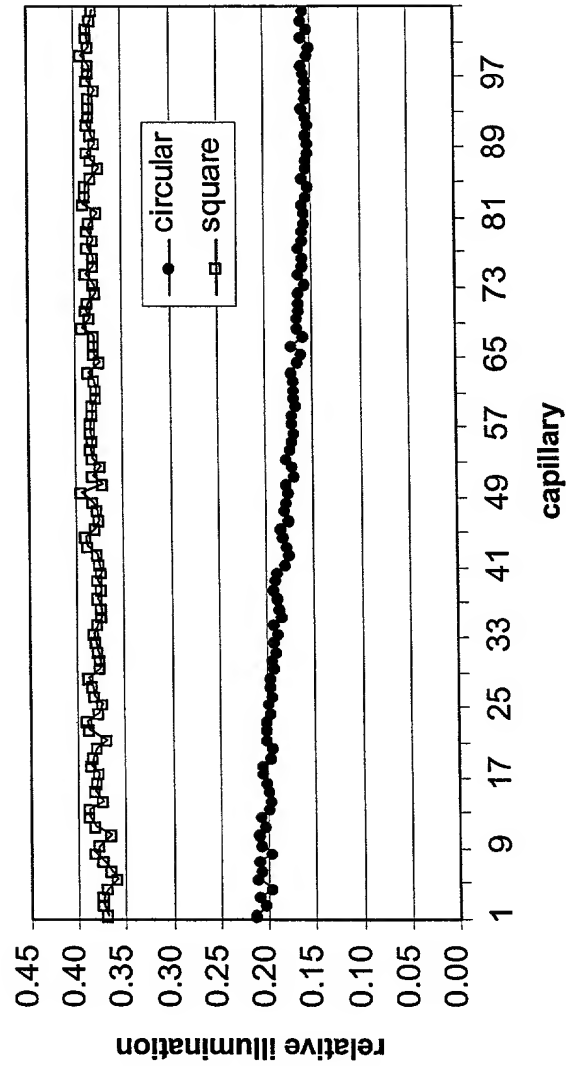


Fig. 22

